

IMPORTANT WARNING WHEN REPLACING A CONTROLLER ON OPxxx, OMAXI, OMINI

On some old osmosers, the cable bundle has no white wire on the 4th pin of the connector.



old cable bundle:

standard OPxxx, OMAXI, OMINI cable bundle:





ANY CABLE BUNDLE WITHOUT WHITE WIRE ON PIN 4 MUST BE REPLACED BEFORE CONNECTING A NEW CONTROLLER !!!

(in such a case, the internal fuse will burn and the osmoser will not work)


CONNECTION OF THE ELECTRIC CABLE BUNDLE

[Original file](#)

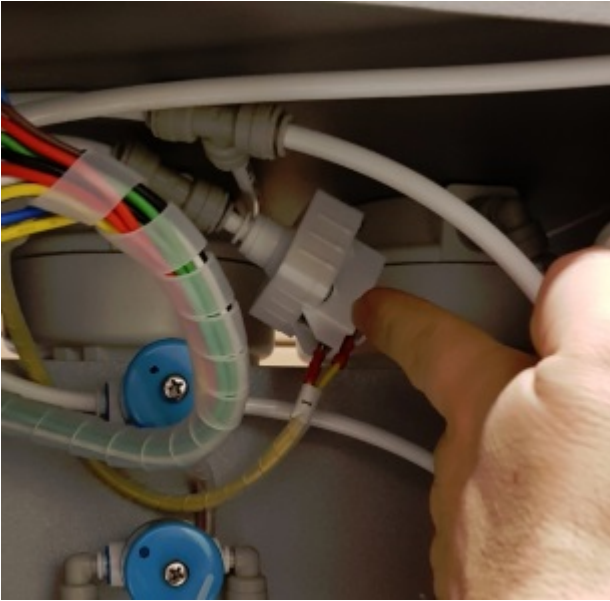


WIRE	CONNECTED TO
Cable 1 Yellow	 <p data-bbox="362 1227 975 1263">Low Pressure Switch</p>
Cable 2 Blue	 <p data-bbox="362 1868 975 1901">Cable connector of the High Pressure Switch</p>

Cable 3 Red

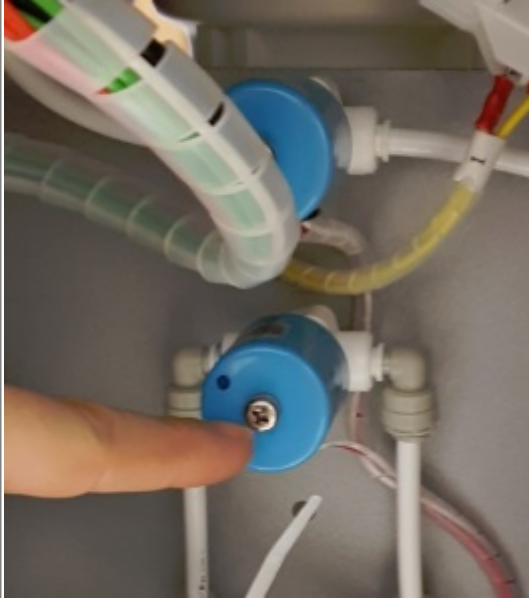


Low Solenoid Valve

**Cable 4 Green
Black**

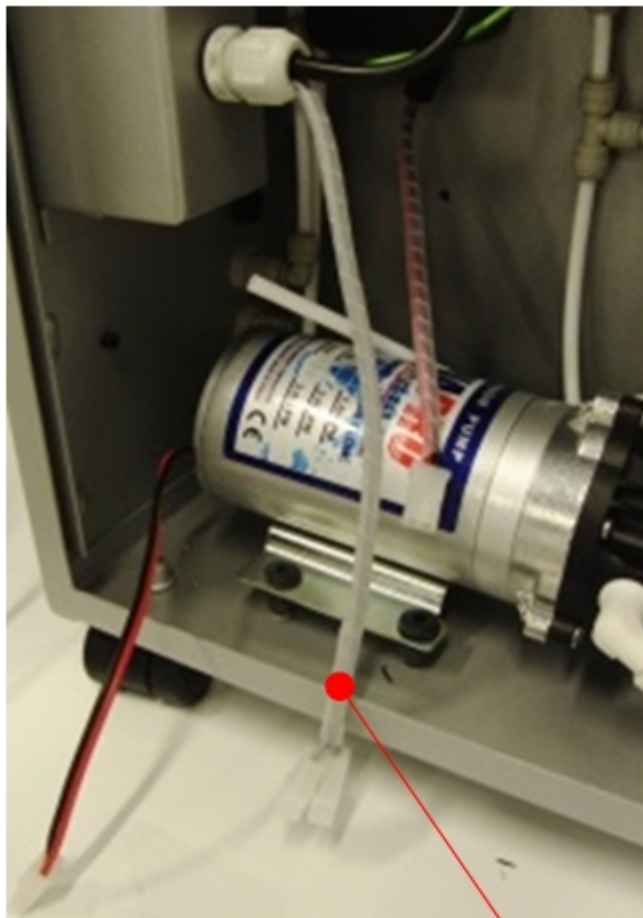


Male connector:
Connected with the
cable ④

Female connector:
Connected with the
booster pump

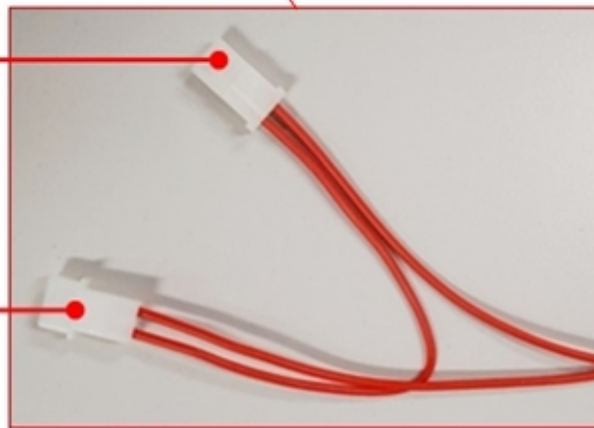

T jonction

**Cable 5 Green
White**

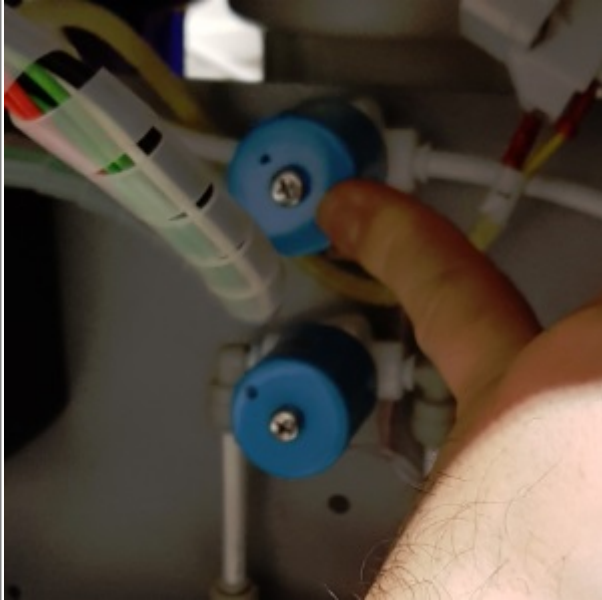

High Solenoid Valve

**Cable 6 Blue
Brown**



24V Power supply

From:

<http://diasys-technologies.com/waterpurifiers/> - **DiaSys Water Purifier Systems**

Permanent link:

http://diasys-technologies.com/waterpurifiers/doku.php?id=replace_controllerwithoutwhitewire

Last update: **2019/11/15 16:09**

